

AFRRI TN71-6

OCTOBER 1971

**AFRRI**  
**TECHNICAL**  
**NOTE**

**AN IMPROVED AUTOMATED METHOD  
FOR PLASMA GLUCOSE ANALYSIS  
WITH HIGH SPECIFICITY AND SENSITIVITY  
IN THE 5 TO 50 MICROGRAM RANGE**

**P. Z. Sobocinski**

**K. M. Hartley**

**W. J. Canterbury**

**ARMED FORCES RADIOBIOLOGY RESEARCH INSTITUTE**  
**Defense Nuclear Agency**  
**Bethesda, Maryland**

---

Approved for public release; distribution unlimited


All aspects of investigative programs involving the use of laboratory animals sponsored by DoD components are conducted according to the principles enunciated in the "Guide for Laboratory Animal Facilities and Care", prepared by the National Academy of Sciences - National Research Council.

AN IMPROVED AUTOMATED METHOD FOR PLASMA GLUCOSE  
ANALYSIS WITH HIGH SPECIFICITY AND SENSITIVITY  
IN THE 5 TO 50 MICROGRAM RANGE

P. Z. SOBOCINSKI  
K. M. HARTLEY  
W. J. CANTERBURY



R. E. GEORGE  
Commander, MSC, USN  
Chairman  
Radiation Biology Department



MYRON I. VARON  
Captain MC USN  
Director

ARMED FORCES RADIOBIOLOGY RESEARCH INSTITUTE  
Defense Nuclear Agency  
Bethesda, Maryland

## TABLE OF CONTENTS

	Page
Abstract . . . . .	ii
I. Introduction . . . . .	1
II. Materials . . . . .	1
III. Procedure . . . . .	2
IV. Results . . . . .	3
References . . . . .	5

## LIST OF FIGURES

Figure 1. Diagram of the flow manifold for the automated determination of glucose . . . . .	2
Figure 2. Color formed by a 5 mg/100 ml glucose solution at various pH values . . . . .	3

## TABLE

Table I. Replicate Glucose Analyses of Two Commercial Control Sera . .	4
--	---

## ABSTRACT

An improved highly sensitive automated procedure for the analysis of plasma glucose in ultramicro sample volumes is presented. The procedure utilizes the glucose oxidase-peroxidase-dye reaction with an extract of gum guaiac as the chromogenic oxygen acceptor. Details for flow manifold construction and reagent composition are presented together with data concerning the precision of the method.

## I. INTRODUCTION

Studies of blood glucose changes after radiation exposure of small laboratory animals produced a requirement for a specific and highly sensitive procedure for glucose analysis in ultramicro sample volumes. Numerous automated methods using the glucose oxidase-peroxidase-dye reaction for the determination of true glucose have been proposed.<sup>1</sup> These methods, however, either lack sufficient sensitivity for the determination of glucose in ultramicro sample volumes or require the use of some form of range expansion on the recording instrument.

A highly sensitive automated method employing an extract of gum guaiac as the chromogenic oxygen acceptor has recently been suggested by Hochella and Hill.<sup>2</sup> In our hands, however, the method yielded poor results which were primarily attributable to their design of the flow manifold. This report describes the modifications in manifold construction and reagent composition which are required to make the procedure usable for assaying plasma glucose in the 5 to 50 microgram range normally encountered in the ultramicro sample volumes obtained from small laboratory animals. The high sensitivity of the chromogen eliminates the need for recorder range expansion.

## II. MATERIALS

The reagents used are those described by Hochella and Hill<sup>2</sup> with the following exceptions:

(a) enzyme: 5 ml of Fermcozyme 952 DM, a mixture of glucose oxidase and peroxidase (Fermco Laboratories, Chicago, Illinois), diluted to 100 ml with distilled water; no preservative is added since the reagent is stable at room temperature;

(b) buffer: 1.0 M sodium acetate, pH 5.2, to which 20 ml of Triton X-100 (Rohm and Haas Company, Philadelphia, Pennsylvania) is added per 1000 ml of buffer. Care should be taken to insure complete mixing of the buffer and Triton X-100.

### III. PROCEDURE

The flow diagram for the procedure using the AutoAnalyzer (Technicon Corporation, Tarrytown, New York) is shown in Figure 1. We have routinely operated the system at a sampling rate of 40 per hour with a water wash between samples to obtain optimum resolution of sample peaks.

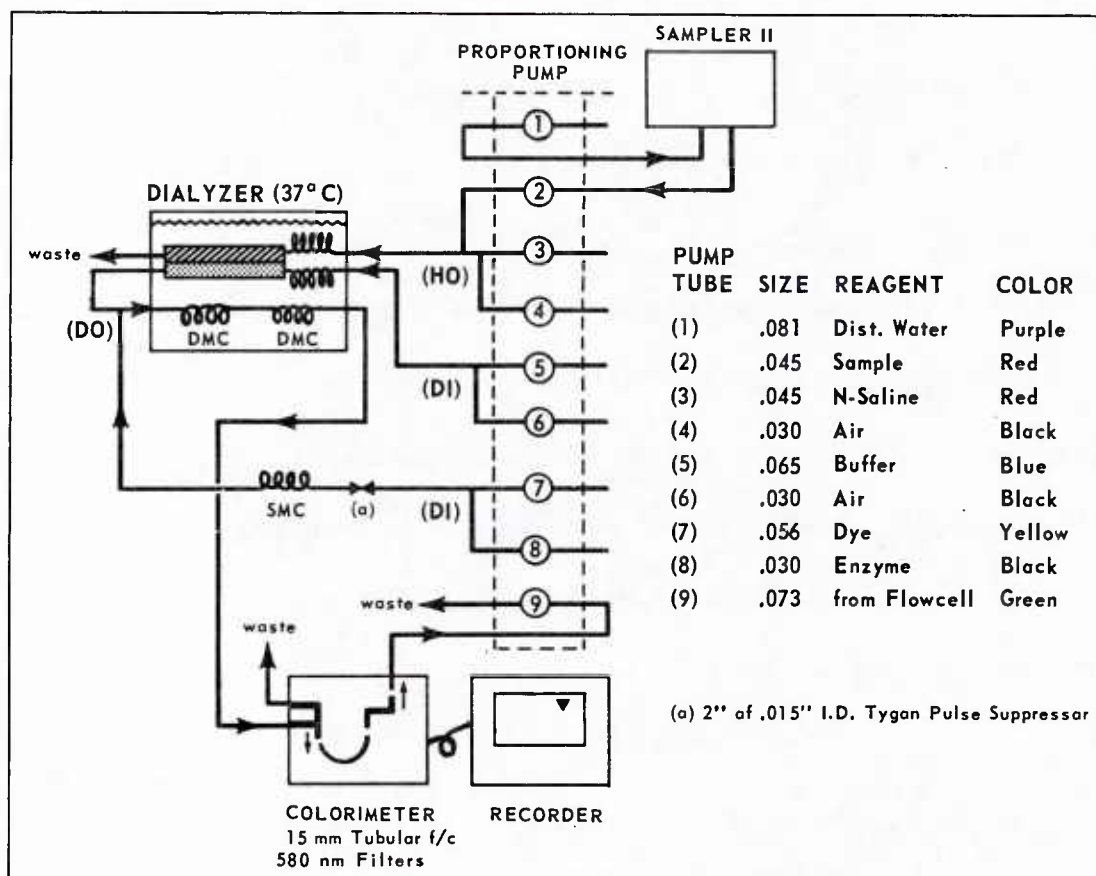


Figure 1. Diagram of the flow manifold for the automated determination of glucose. Glass fittings (Bulletin GF3, Technicon Corporation) and tube sizes are Technicon designations.

Before analysis, each sample must be diluted to a final volume of at least 1 ml to accommodate the volume of aspirated sample. We routinely make a 1 to 50 dilution with a 0.9 percent (w/v) aqueous solution of sodium chloride using a Fisher 240 diluter (Fisher Scientific Company, Pittsburgh, Pennsylvania).

#### IV. RESULTS

The sensitivity of the method is 0.210 O.D. units per 10  $\mu$ g glucose. The optimum pH for the reaction mixture was found to be approximately 5.2. However, as shown in Figure 2, the sensitivity is not appreciably affected within the pH range 5.0 to 5.6.

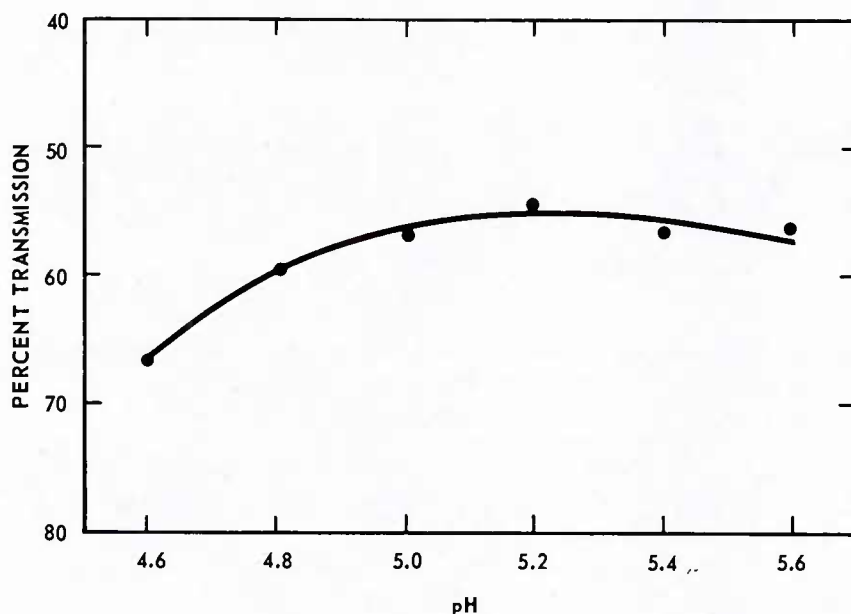


Figure 2. Color formed by a 5 mg/100 ml glucose solution at various pH values

Results of replicate analyses performed on two commercial control sera shown in Table I indicate that the dilution procedure does not affect the precision of the method. The standard deviation for the procedure is 2 mg/100 ml.



Table I. Replicate Glucose Analyses of Two Commercial Control Sera

Assay* #	Glucose (mg/100 ml)	
	Control A†	Control B‡
1	97.5	220.0
2	100.0	225.0
3	100.0	225.0
4	97.5	225.0
5	95.0	225.0
6	100.0	225.0
7	97.5	220.0
8	95.0	225.0
9	100.0	223.0
10	97.5	225.0
11	97.5	220.0
12	97.5	223.0
13	97.5	223.0
14	97.5	223.0
Mean	97.9	223.4
S. D.	1.7	2.0
Manufacturer's assay (method)	103 ± 5 (glucose oxidase, Hyland)	228 ± 10 (Nelson-Somogyi)

\* Separate 1 to 50 aqueous dilutions (see text)

† Hyland Lot 0369D040A1, Hyland Division Travenol Laboratories, Inc., Los Angeles, California

‡ Moni-trol II Lot PTD-21 C.D., Dade Division, American Hospital Supply Corporation, Miami, Florida

Neither ascorbic acid, uric acid, nor reduced glutathione in physiological concentrations was found to interfere with the procedure.

## REFERENCES

1. Faulkner, D. E. An automated micro determination of blood-glucose with the AutoAnalyzer. *Analyst* 90:736-744, 1965.
2. Hochella, N. J. and Hill, J. B. The collection and preservation of blood on filter paper for blood glucose determinations. In: *Automation in Analytical Chemistry*, Technicon Symposia, 1967, Vol. I, pp. 3-6. White Plains, New York, Mediad Incorporated, 1968.

## DISTRIBUTION LIST

### AIR FORCE

The Surgeon General, U. S. Department of the Air Force, Washington, D. C. 20314 (1)  
Executive Officer, Director of Professional Services, Office of the Surgeon General, Hq. USAF (AFMSPA),  
Washington, D. C. 20314 (1)  
Headquarters, U. S. Air Force (AFMSPAB), Washington, D. C. 20314 (1)  
Chief, Weapons and Weapons Effects Division, Hq. RTD (RTTW), Bolling AFB, Washington, D. C. 20332 (1)  
Office of the Command Surgeon (ADCSG), Hq. ADC, USAF, Ent AFB, Colorado 80912 (1)  
Air Force Weapons Laboratory, ATTN: WLIL (1), ATTN: WLRB-2 (1), Kirtland AFB, New Mexico 87117 (2)  
Chief, Nuclear Medicine Department, P. O. Box 5088, USAF Hospital, Wright-Patterson AFB, Ohio 45433 (1)  
USAFSAM (RA), ATTN: Chief, Radiobiology Division, Brooks AFB, Texas 78235 (1)  
USAFSAM, ATTN: EDAD, Brooks AFB, Texas 78235 (1)

### ARMY

The Surgeon General, U. S. Department of the Army, Washington, D. C. 20314 (1)  
Surgeon General, ATTN: MEDDH-N, U. S. Department of the Army, Washington, D. C. 20314 (1)  
USACDC CSSG, Doctrine Division, Fort Lee, Virginia 23801 (1)  
Commanding Officer, USACDC CBR Agency, Fort McClellan, Alabama 36201 (1)  
Commanding Officer, U. S. Army Combat Developments Command, Institute of Nuclear Studies, Fort Bliss, Texas  
79916 (1)  
CG, USCONARC, ATTN: ATUTR-TNG (NBC), Fort Monroe, Virginia 23351 (1)  
Nuclear Branch AMCRD-DN-RE, U. S. Army Materiel Command, Washington, D. C. 20315 (1)  
Commanding Officer, U. S. Army Medical Research Laboratory, Fort Knox, Kentucky 40121 (1)  
Commanding Officer, USA Nuclear Medical Research Detachment, Europe, APO New York, N. Y. 09180 (2)  
Chief of Research and Development, ATTN: Nuclear, Chemical and Biological Division, U. S. Department of the  
Army, Washington, D. C. 20310 (1)  
Army Research Office, ATTN: Chief, Scientific Analysis Branch, Life Sciences Division, 3045 Columbia Pike,  
Arlington, Virginia 22204 (1)  
Division of Nuclear Medicine, Walter Reed Army Institute of Research, Walter Reed Army Medical Center,  
Washington, D. C. 20012 (5)  
Commanding Officer, U. S. Army Environmental Hygiene Agency, ATTN: USAEHA-RP, Edgewood Arsenal, Mary-  
land 21010 (1)  
Commandant, U. S. Army Medical Field Service School, ATTN: MEDEW-ZNW, Fort Sam Houston, Texas 78234 (1)

### NAVY

Chief, Bureau of Medicine and Surgery, U. S. Navy Department, Washington, D. C. 20390 (1)  
Chief, Bureau of Medicine and Surgery, ATTN: Code 71, U. S. Navy Department, Washington, D. C. 20390 (1)  
Commanding Officer, Naval Aerospace Medical Institute, Naval Aviation Medical Center, ATTN: Director of  
Research, Pensacola, Florida 32512 (3)  
Commanding Officer, Nuclear Weapons Training Center, Atlantic, Nuclear Warfare Department, Norfolk, Virginia  
23511 (1)  
Commanding Officer, Nuclear Weapons Training Center, Pacific, U. S. Naval Air Station, North Island, San Diego,  
California 92135 (1)  
Director, Biological Sciences Division, Office of Naval Research, Washington, D. C. 20360 (1)  
Commanding Officer, U. S. Naval Hospital, ATTN: Director, REEL, National Naval Medical Center, Bethesda,  
Maryland 20014 (1)  
Head, Animal Behavioral Sciences Branch, Naval Aerospace Medical Institute, Naval Aerospace Medical Center,  
ATTN: Dr. John S. Thach, Jr., Pensacola, Florida 32512 (1)  
Commanding Officer, Naval Submarine Medical Center, Naval Submarine Base, NL, ATTN: Medical Library,  
Groton, Connecticut 06340 (1)  
Commanding Officer, Naval Submarine Medical Center, Naval Submarine Base, NL, ATTN: Code 53, Nuclear Medi-  
cine Training Division, Groton, Connecticut 06340 (1)

### D. O. D.

Director, Defense Nuclear Agency, Washington, D. C. 20305 (1)  
Director, Defense Nuclear Agency, ATTN: DDST, Washington, D. C. 20305 (1)  
Director, Defense Nuclear Agency, ATTN: Chief, Medical Directorate, Washington, D. C. 20305 (4)  
Director, Defense Nuclear Agency, ATTN: Chief, Radiation Directorate, Washington, D. C. 20305 (1)

D.O.D. (continued)

Director, Defense Nuclear Agency, ATTN: Technical Library (APTL), Washington, D. C. 20305 (2)  
Commanding Officer, Harry Diamond Laboratories, ATTN: Nuclear Vulnerability Branch, Washington, D. C.  
20438 (1)  
Commander, Field Command, Defense Nuclear Agency, ATTN: FC Technical Library, Kirtland AFB, New Mexico  
87117 (1)  
Commander, Headquarters Field Command, Defense Nuclear Agency, ATTN: FCTG8, Kirtland AFB, New Mexico  
87117 (2)  
Director, Armed Forces Institute of Pathology, Washington, D. C. 20305 (1)  
Administrator, Defense Documentation Center, Cameron Station, Bldg. 5, Alexandria, Virginia 22314 (12)

OTHER GOVERNMENT

U. S. Atomic Energy Commission, Headquarters Library, Reports Section, Mail Station G-17, Washington, D. C.  
20545 (1)  
U. S. Atomic Energy Commission, Division of Biology and Medicine, Washington, D. C. 20545 (1)  
U. S. Atomic Energy Commission, Bethesda Technical Library, 7920 Norfolk Avenue, Bethesda, Maryland 20014 (1)  
National Aeronautics and Space Administration, ATTN: Lt. Col. Charles M. Barnes, USAF, DB-3, MSC, Houston,  
Texas 77058 (1)  
National Aeronautics and Space Administration, Manned Spacecraft Center, ATTN: Dr. B. D. Newsom, Mail Code  
DA, Houston, Texas 77058 (1)  
National Bureau of Standards, ATTN: Chief, Radiation Physics Division, Washington, D. C. 20234 (1)  
U. S. Public Health Service, Bureau of Radiological Health, Division of Biological Effects, 12720 Twinbrook Park-  
way, Rockville, Maryland 20852 (1)  
U. S. Public Health Service, Bureau of Radiological Health, Library, 12720 Twinbrook Parkway, Rockville, Mary-  
land 20852 (1)  
U. S. Public Health Service, Northeastern Radiological Health Laboratory, 109 Holton Street, Winchester, Massa-  
chusetts 01890 (1)  
U. S. Public Health Service, Southeastern Radiological Health Laboratory, P. O. Box 61, Montgomery, Alabama  
36101 (1)  
U. S. Public Health Service, Southwestern Radiological Health Laboratory, P. O. Box 15027, Las Vegas, Nevada  
89114 (1)

OTHER

Argonne National Laboratory, Library Services Department, Report Section Bldg. 203, RM-CE-125, 9700 South  
Cass Avenue, Argonne, Illinois 60440 (1)  
Dr. Donald G. Baker, Radiobiology Department, Zellerbach Saroni Tumor Institute, 1600 Divisadero Street,  
San Francisco, California 94115 (1)  
Dr. J. T. Brennan, Radiology Department, University of Pennsylvania, 3400 Spruce Street, Philadelphia, Pennsyl-  
vania 19104 (1)  
Brookhaven National Laboratory, Information Division, ATTN: Research Library, Upton, Long Island, New York  
11973 (2)  
Dr. J. S. Burkle, Director of Nuclear Medicine, York Hospital, York, Pennsylvania 17403 (1)  
S. C. Bushong, Department of Radiology, Baylor University College of Medicine, Houston, Texas 77024 (1)  
University of California, Lawrence Radiation Laboratory, Library, Bldg. 50, Room 134, Berkeley, California  
94720 (1)  
Director, Radiobiology Laboratory, University of California, Davis, California 95616 (1)  
University of California, Lawrence Radiation Laboratory, Technical Information Division Library L-3, P. O. Box  
808, Livermore, California 94551 (2)  
University of California, Laboratory of Nuclear Medicine and Radiation Biology, Library, 900 Veteran Avenue,  
Los Angeles, California 90024 (1)  
Dr. C. Jelleff Carr, Director, Life Sciences Research Office, Federation of American Societies for Experimental  
Biology, 9650 Rockville Pike, Bethesda, Maryland 20014 (1)  
Cdr. William H. Chapman, USN (Ret.), Bio-Medical Division L-523, Lawrence Radiation Laboratory, University of  
California, P. O. Box 808, Livermore, California 94551 (1)  
Director, Collaborative Radiological Health Laboratory, Colorado State University, Fort Collins, Colorado 80521 (1)  
Dr. L. W. Davis, Radiology Department, University of Pennsylvania, 3400 Spruce Street, Philadelphia, Pennsyl-  
vania 19104 (1)  
Professor Merrill Eisenbud, New York University, Tuxedo, New York 10987 (1)  
Dr. T. C. Evans, Radiation Research Laboratory, College of Medicine, University of Iowa, Iowa City, Iowa 52240 (1)

## OTHER (continued)

Dr. Arnold Feldman, Institute of Radiology, School of Medicine, Washington University, 510 South Kingshighway, St. Louis, Missouri 63110 (1)

Mr. Orin Gelderloos, Division of Literature, University of Michigan, Dearborn Campus, Dearborn, Michigan 48124 (1)

General Dynamics/Fort Worth, ATTN: Librarian, P. O. Box 748, Fort Worth, Texas 76101 (1)

Gulf General Atomic Incorporated, ATTN: Library, P. O. Box 608, San Diego, California 92112 (1)

Dr. James E. Huff, Department of Pharmacology and Toxicology, School of Medicine and Dentistry, University of Rochester, 260 Crittenden Blvd., Rochester, New York 14620 (1)

IIT Research Institute, ATTN: Document Library, 10 West 35th Street, Chicago, Illinois 60616 (1)

Johns Hopkins University, Applied Physics Laboratory, ATTN: Document Library, 8621 Georgia Avenue, Silver Spring, Maryland 20910 (1)

Dr. R. F. Kallman, Department of Radiology, Stanford University, Palo Alto, California 94305 (1)

Dr. L. S. Kelly, Donner Laboratory, University of California at Berkeley, Berkeley, California 94720 (1)

Dr. Robert Landolt, Bionucleonics Department, Purdue University, Lafayette, Indiana 47907 (1)

Los Alamos Scientific Laboratory, ATTN: Report Librarian, P. O. Box 1663, Los Alamos, New Mexico 87544 (1)

Director, Nuclear Science Center, Louisiana State University, Baton Rouge, Louisiana 70803 (2)

Lovelace Foundation for Medical Education and Research, Document Library, 5200 Gibson Blvd., S. E., Albuquerque, New Mexico 87108 (1)

Dr. Ross A. McFarland, Guggenheim Professor of Aerospace Health and Safety, Harvard School of Public Health, 665 Huntington Avenue, Boston, Massachusetts 02115 (1)

Dr. J. I. Marcum, Rand Corporation, 1700 Main Street, Santa Monica, California 90401 (1)

Massachusetts Institute of Technology, M.I.T. Libraries, Technical Reports, Room 14 E-210, Cambridge, Massachusetts 02139 (1)

Dr. Charles W. Mays, Physics Group Leader, Radiobiology Division, University of Utah, Salt Lake City, Utah 84112 (1)

Ohio State University, Nuclear Reactor Laboratory, 1298 Kinnear Road, Columbus, Ohio 43212 (1)

Dr. Harvey M. Patt, Laboratory of Radiobiology, University of California, San Francisco Medical Center, San Francisco, California 94122 (1)

Purdue University, Nuclear Engineering Library, Lafayette, Indiana 47907 (1)

Dr. S. M. Reichard, Director, Division of Radiobiology, Medical College of Georgia, Augusta, Georgia 30902 (1)

Dr. H. H. Rossi, 630 West 168th Street, New York, N. Y. 10032 (1)

Dr. Eugene L. Saenger, Director, Radioisotope Laboratory, Cincinnati General Hospital, Cincinnati, Ohio 45229 (1)

Sandia Corporation Library, P. O. Box 5800, Albuquerque, New Mexico 87115 (1)

Scientific Committee on the Effects of Atomic Radiation, ATTN: Library, United Nations Room 3267, United Nations Plaza, New York, N. Y. 10017 (1)

Scope Publications, Franklin Station, P. O. Box 7407, Washington, D. C. 20004 (1)

Texas A and M University, Radiation Biology Laboratory, Texas Engineering Experiment Station, College Station, Texas 77840 (2)

Texas Nuclear Corporation, ATTN: Director of Research, Box 9267 Allandale Station, Austin, Texas 78756 (1)

University of Rochester, Atomic Energy Project Library, P. O. Box 287, Station 3, Rochester, New York 14620 (1)

University of Southern California, Nuclear Physics Laboratory, University Park, Los Angeles, California 90007 (1)

Western Reserve University, Department of Radiology, Division of Radiation Biology, Cleveland, Ohio 44106 (1)

Mr. Lionel Zamore, 601 Brightwater Court, Brooklyn, New York 11235 (1)

## FOREIGN

International Atomic Energy Agency, Kärrntnerring 11, Vienna I. 1010, Austria (1)

European Atomic Energy Community, C. E. E. A., Library, 51 rue Belliard, Brussels 4, Belgium (1)

Dr. L. G. Lajtha, Paterson Laboratories, Christie Hospital and Holt Radium Institute, Manchester, England (1)

Dr. L. F. Lamerton, Biophysics Department, Institute of Cancer Research, Surrey Branch, Belmont, Sutton, Surrey, England (1)

National Lending Library for Science and Technology, Boston Spa, Yorkshire, England (1)

Directorate of Medical and Health Services, FAF (Federal Armed Forces), Bonn, Ermekeilstrasse 27, West Germany (1)

Abteilung für Strahlenbiologie im Institut für Biophysik der Universität Bonn, 53 Bonn-Venusberg, Annaberger Weg 15, Federal Republic of Germany (2)

Prof. Dr. H. Langendorff, Direktor des Radiologischen Instituts der Universität, 78 Freiburg im Breisgau, Albertstrasse 23, Germany (1)



FOREIGN (continued)

- Priv.-Doz. Dr. O. Messerschmidt, Radiologisches Institut der Universität, 78 Freiburg im Breisgau, Albertstrasse 23, Germany (1)
- Dr. Helmut Mitschrich, Akademie des Sanitäts- und Gesundheitswesens der Bundeswehr, Spezialstab ATV, 8 München, Schwere Reiterstrasse 4, Germany (2)
- Prof. Dr. F. Wachsmann, Gesellschaft für Strahlenforschung m.b.H., 8042 Neuherberg bei München, Institut für Strahlenschutz, Ingolstadter Landstrasse 1, München, Germany (1)
- Dr. M. Feldman, Section of Cell Biology, The Weizmann Institute of Science, Rehovoth, Israel (1)
- Dr. G. W. Barendsen, Radiobiological Institute TNO, Rijswijk, Netherlands (1)
- Dr. L. M. van Putten, Radiobiological Institute TNO, 151 Lance Kleiweg, Rijswijk 2 H, Netherlands (1)
- Puerto Rico Nuclear Center, ATTN: Reading Room, College Station, Mayaguez, Puerto Rico 00708 (2)
- Dr. H. Cottier, Pathological Institut der Universität, Bern, Switzerland (1)

DOCUMENT CONTROL DATA - R & D

(Security classification of title, body of abstract and indexing annotation must be entered when the overall report is classified)

1. ORIGINATING ACTIVITY (Corporate author) Armed Forces Radiobiology Research Institute Defense Nuclear Agency Bethesda, Maryland 20014		2a. REPORT SECURITY CLASSIFICATION UNCLASSIFIED	
		2b. GROUP N/A	
3. REPORT TITLE  AN IMPROVED AUTOMATED METHOD FOR PLASMA GLUCOSE ANALYSIS WITH HIGH SPECIFICITY AND SENSITIVITY IN THE 5 TO 50 MICROGRAM RANGE			
4. DESCRIPTIVE NOTES (Type of report and inclusive dates)			
5. AUTHOR(S) (First name, middle initial, last name)  P. Z. Sobocinski, K. M. Hartley and W. J. Canterbury			
6. REPORT DATE October 1971		7a. TOTAL NO. OF PAGES 11	7b. NO. OF REFS 2
8a. CONTRACT OR GRANT NO.		9a. ORIGINATOR'S REPORT NUMBER(S)  AFRRI TN71-6	
b. PROJECT NO. NWER XAXM			
c. Task and Subtask C 901		9b. OTHER REPORT NO(S) (Any other numbers that may be assigned this report)	
d. Work Unit 03			
10. DISTRIBUTION STATEMENT  Approved for public release; distribution unlimited			
11. SUPPLEMENTARY NOTES		12. SPONSORING MILITARY ACTIVITY Director Defense Nuclear Agency Washington, D. C. 20305	
13. ABSTRACT  An improved highly sensitive automated procedure for the analysis of plasma glucose in ultramicro sample volumes is presented. The procedure utilizes the glucose oxidase-peroxidase-dye reaction with an extract of gum guaiac as the chromogenic oxygen acceptor. Details for flow manifold construction and reagent composition are presented together with data concerning the precision of the method.			

UNCLASSIFIED

Security Classification

14.

KEY WORDS

LINK A

LINK B

LINK C

ROLE

WT

ROLE

WT

ROLE

WT

UNCLASSIFIED

Security Classification